

Cardiac

ichroma™ Myoglobin Neo

INTENDED USE

ichroma™ Myoglobin Neo is a fluorescence immunoassay (FIA) for the quantitative determination of Myoglobin in human whole blood/serum/plasma. It is useful as an aid in management and monitoring of acute myocardial infarction (AMI).

For *in vitro* diagnostic use only.

INTRODUCTION

Myoglobin is an iron- and oxygen-binding protein found in both skeletal and myocardial muscles. It acts as a transport protein and is involved in diffusion of oxygen in the muscle tissue. Myoglobin is a single-chain globular protein of 154 amino acids. It is composed of a central iron-containing 'Heme' which is enclosed in a compact bundle-like or prism-like arrangement formed by the eight right-handed α -helices^{1,2}. Being a cytoplasmic protein having low molecular weight (of 17,699 daltons), myoglobin is released into the serum more rapidly as compared to other cardiac markers upon damage to the myocardial cells. Serum concentration of myoglobin increases above the normal range as early as 1 hour after acute myocardial infarction (AMI), attains peak level in approximately 4 to 8 hours after the onset and normalize rapidly afterwards. Thus myoglobin is better suited as a cardiac marker for early diagnosis of AMI. However, the elevated myoglobin is not specific to AMI owing to its large quantities in skeletal muscles as well. Despite its low clinical specificity and weak predictive value towards AMI, myoglobin is still a promising cardiac marker when other markers such as Creatin Kinase Isoenzyme-MB (CK-MB) and Cardiac Troponin-I (cTn-I) as well as other indicators like clinical signs and ECG are taken into account for diagnosis/confirmation of AMI³⁻⁸.

PRINCIPLE

The test uses a sandwich immunodetection method.

The detector antibodies in buffer bind to antigens in the sample, forming antigen-antibody complexes, and migrate onto nitrocellulose matrix to be captured by the other immobilized antibodies on a test strip.

More antigens in the sample will form more antigen-antibody complexes which lead to stronger fluorescence signal by detector antibodies, which is processed by the instrument for ichroma™ tests to show myoglobin concentration in the sample.

COMPONENTS

ichroma™ Myoglobin Neo consists of 'cartridges', 'detector tubes' and 'detector diluent'.

- The cartridge contains the membrane called a test strip which has anti-myoglobin at the test line and streptavidin at the control line. All cartridges are individually sealed in an aluminum foil pouch containing a desiccant, and they are further packaged in a box.
- The detector tube has a granule containing myoglobin-fluorescence conjugate, biotin-BSA-fluorescence conjugate and sodium azide as a preservative in Tris-Cl buffer. All detector tubes are packed in a pouch.
- The detector diluent contains tween 20, sodium azide as a preservative in phosphate buffered saline (PBS), and it is pre-dispensed in a vial. The detector diluent is packed in a box.

WARNINGS AND PRECAUTIONS

- For *in vitro* diagnostic use only.
- Follow the instructions and procedures described in this 'Instructions for use'.
- Use only fresh samples and avoid direct sunlight.
- Lot numbers of all the test components (cartridge, detector tube, detector diluent and ID chip) must match each other.
- Do not interchange the test components between different lots or use the test components after the expiration date, either of which might yield incorrect test result(s).
- Do not reuse cartridges or detector tubes. A cartridge tube should be used for testing one sample only. A detector tube should be used for processing of one sample only.
- The cartridge should remain sealed in its original pouch until just before use. Do not use cartridge, if pouch is damaged or has already been opened.
- Frozen sample should be thawed only once. For shipping, samples must be packed in accordance with local regulations. Sample with severe hemolysis and/or hyperlipidemia must not be used.
- If test components and/or sample are stored in refrigerator, then allow cartridge, detector tube, detector diluent and sample to be at room temperature for approximately 30 minutes before use.
- The instrument for ichroma™ tests may generate slight vibration during use.
- Used cartridges, detector tubes, detector diluent, capillary tube and pipette tips should be handled carefully and discarded by an appropriate method in accordance with relevant local regulations.
- The detector tube and the detector diluent contain sodium azide (NaN₃), and it may cause certain health issues like convulsions, low blood pressure, low heart rate, loss of consciousness, lung injury and respiratory failure. Avoid contact with skin, eyes, and clothing. In case of contact, rinse immediately with running water.
- No Biotin interference was observed in ichroma™

Myoglobin Neo when biotin concentration in the sample was below 200 ng/mL. If a patient has been taking biotin at dosage of more than 0.03 mg a day, it is recommended to test again 24 hours after discontinuation of biotin intake.

■ **ichroma™ Myoglobin Neo** will provide accurate and reliable results subject to the below conditions.

- **ichroma™ Myoglobin Neo** should be used only in conjunction with the instrument for ichroma™ tests.
- Have to use recommended anticoagulant.

Recommended anticoagulant

K₃ EDTA, Lithium heparin, Sodium citrate

LIMITATION OF THE TEST SYSTEM

- The test may yield false positive result(s) due to the cross-reactions and/or non-specific adhesion of certain sample components to the capture/detector antibodies.
- The test may yield false negative result(s) due to the non-responsiveness of the antigens to the antibodies which is the most common if the epitope is masked by some unknown components, so therefore not being able to be detected or captured by the antibodies. The instability or degradation of the antigens with time and/or temperature may also cause false negative result as it makes the antigens unrecognizable by the antibodies.
- Other factors may interfere with the test and cause erroneous results, such as technical/procedural errors, degradation of the test components/reagents or presence of interfering substances in the test samples.
- Any clinical diagnosis based on the test result must be supported by a comprehensive judgment of the concerned physician in conjunction with clinical symptoms and other relevant test results.

STORAGE AND STABILITY

Storage condition			
Component	Storage Temperature	Shelf life	Note
Cartridge	2 ~ 30°C	20 months	Disposable
Detector tube	2 ~ 30°C	20 months	Disposable
Detector diluent	2 ~ 30°C	20 months	Unopened
		20 months	Opened

- After the cartridge pouch is opened, the test should be performed immediately.

MATERIALS SUPPLIED

REF CFPC-151

Components of **ichroma™ Myoglobin Neo**

- Cartridge box:
 - Cartridge 25
 - Detector tube 25
 - Detector diluent 1
 - ID chip 1
 - Instructions for use 1

MATERIALS REQUIRED BUT SUPPLIED ON DEMAND

Following items can be purchased separately with **ichroma™ Myoglobin Neo**.

Please contact our sales division for more information.

■ **Instrument for ichroma™ tests**

- **ichroma™ II** REF FPRR021
- **ichroma™ III** REF FPRR037
- **ichroma™ M3** REF FPRR035
- **ichroma™ 50 plus** REF FPRR036
- **Boditech Myoglobin Control** REF CFPO-244
- **Boditech Cardiac Control** REF CFPO-98

SAMPLE COLLECTION AND PROCESSING

The sample type for **ichroma™ Myoglobin Neo** is human whole blood/serum/plasma.

- It is recommended to test the sample within 24 hours after collection when collected sample is stored at room temperature.
- The samples (serum, plasma) should be separated from the clot by centrifugation within 3 hours after the collection of whole blood.
- The samples (whole blood, serum, plasma) may be stored for a week at 2-8°C prior to being tested. If testing will be delayed more than a week, samples (serum, plasma) should be frozen at -20°C.
- The samples (serum, plasma) stored frozen at -20°C for 3 months showed no performance difference.
- However, the whole blood sample should not be kept in a freezer in any case.
- As a repeated freeze-thaw cycle may affect the test result, do not refreeze previously frozen samples.

TEST SETUP

- Check the contents of **ichroma™ Myoglobin Neo**: Sealed cartridges, detector tubes, a detector diluent, an ID chip and an instructions for use.
- Ensure that the lot number of the cartridge matches that of the detector tube, the detector diluent as well as an ID chip.
- If the sealed cartridge, the detector tube and the detector diluent have been stored in a refrigerator, place them on a clean and flat surface at room temperature for at least 30 minutes before testing.
- Turn on the instrument for **ichroma™** tests.
- Insert the ID chip into the 'ID chip port'.
- ※ **Please refer to the instrument for ichroma™ tests operation manual for complete information and operating instructions**

TEST PROCEDURE

► ichroma™ II, ichroma™ M3

Multi test mode

1) Take 150 μ L of detector diluent using a pipette and dispense it to the detector tube containing a granule. When the granule form is completely dissolved in the tube, it becomes detection buffer.
(The detection buffer must be used immediately. Do not exceed 30 seconds.)

2) Take 10 μ L of sample (Human whole blood/serum/plasma/urine) using a pipette and dispense it to the detector tube.

3) Close the lid of the detector tube and mix the sample thoroughly by shaking it about 10 times.
(The sample mixture must be used immediately. Do not exceed 30 seconds.)

4) Take 75 μ L of the sample mixture and dispense it into the sample well of the cartridge.

5) Leave the cartridge at room temperature for 12 minutes.

⚠ Scan the sample-loaded cartridge immediately when the incubation time is over. If not, it will cause inaccurate test result.

6) To scan the sample-loaded cartridge, insert it into the cartridge holder of the instrument for ichroma™ tests. Ensure proper orientation of the cartridge before pushing it all the way inside the cartridge holder. An arrow is marked on the cartridge especially for this purpose.

7) Tap the 'Start' button on the instrument for ichroma™ tests to start the scanning process.
(ichroma™ M3 will start the test automatically after inserting.)

8) The instrument for ichroma™ tests will start scanning the sample-loaded cartridge immediately.

9) Read the test result on the display screen of the instrument for ichroma™ tests.

Single test mode

1) The test procedure is same with the 'Multi test mode 1) – 4)'.

2) Insert the sample-loaded cartridge into the holder of the instrument for ichroma™ tests. Ensure proper orientation of the cartridge before pushing it all the way inside the cartridge holder. An arrow is marked on the cartridge especially for this purpose.

3) Tap the 'Start' button on the instrument for ichroma™ tests.
(ichroma™ M3 will start the test automatically after inserting.)

4) The cartridge goes inside the instrument for ichroma™ tests and will automatically start scanning the sample-loaded cartridge after 12 minutes.

5) Read the test result on the display screen of the instrument for ichroma™ tests.

► ichroma™ III

1) The test procedure is same with the 'Single test mode'.

► ichroma™-50 Plus

1) Insert the tip array in the tip station.

2) Insert the detector tube in the reagent station and cover the reagent station to hold the detector tubes in place.

3) Open the lid of the detector diluent and insert the detector diluent in the diluent station.

4) Insert the cartridge magazine with the cartridges into the magazine station.

5) Insert the sample tube into the blood collection tube rack and load the blood collection tube rack into the sampling station (loading part).

6) Tap the button located in the upper side of the No. of test cartridge region to select the ID chip that you want to use.

7) When the selected cartridge slot is activated, set the number of the detector tube by tapping.

8) Set the number of pipette tips by tapping.

9) Tap the 'Start' button on the left upper of the main screen to start test.

INTERPRETATION OF TEST RESULT

■ The instrument for ichroma™ tests calculates the test result automatically and displays myoglobin concentration of the test sample in terms of ng/mL.

■ Reference value: 70 ng/mL.

■ Working range: 5-500 ng/mL.

QUALITY CONTROL

■ Quality control tests are a part of the good testing practice to confirm the expected results and validity of the assay and should be performed at regular intervals.

■ Quality control tests should also be performed whenever there is any question concerning the validity of the test results.

■ Control materials are provided on demand with ichroma™ Myoglobin Neo. For more information regarding obtaining the control materials, contact [Boditech Med Inc.'s Sales Division for assistance](#).
(Please refer to the Instructions for use of control material.)

PERFORMANCE CHARACTERISTICS

■ Analytical sensitivity

- Limit of Blank (LoB)	1.5 ng/mL
- Limit of Detection (LoD)	3.07 ng/mL
- Limit of Quantitation (LoQ)	5.0 ng/mL

■ Analytical specificity

- Cross-reactivity
Biomolecules listed in the following table were added to the test sample(s) at concentrations much higher than their normal physiological levels in the blood. **ichroma™ Myoglobin Neo** test results did not show any significant cross-reactivity with these biomolecules.

Cross-reactants	Concentration
CK-MB	1,000 ng/mL
NT-proBNP	1,000 ng/mL
Myoglobin	1,000 ng/mL
D-Dimer	1,000 ng/mL

- Interference
Interferents listed in the following table were added to the test sample at the concentration mentioned below. **ichroma™ Myoglobin Neo** test results did not show any significant interference with these materials.

Interferents	Concentration
D-glucose	55.5 mmol/L
L-Ascorbic acid	175 μmol/L
Bilirubin (unconjugated)	684 μmol/L
Hemoglobin	10 g/L
Cholesterol	10.3 mmol/L
Triglyceride	16.94 mmol/L
Lithium Heparin	330 U/dL
K ₃ EDTA	3.4 μmol/L
Sodium citrate	2 mg/mL

■ Precision

- Single site study
Repeatability (within-run precision)
within-laboratory precision (Total precision)
Lot to lot precision
3 Lots of **ichroma™ Myoglobin Neo** were tested for 20 days. Each standard material was tested 2 times per day. For each test, each material was duplicated.

Single-site study						
Myoglobin Neo [ng/mL]	Repeatability		within-laboratory precision		Lot to lot precision	
	AVG [ng/mL]	CV (%)	AVG [ng/mL]	CV (%)	AVG [ng/mL]	CV (%)
55	56.00	5.80	55.52	5.97	55.06	6.02
100	98.18	5.93	99.05	5.79	99.25	5.84
300	299.69	6.79	300.67	6.43	300.41	6.16

- Multi-site study
Reproducibility
1 Lot of **ichroma™ Myoglobin Neo** was tested for 5 days in 3 different sites (1 person per 1 site, 1 instrument per 1 site). Each standard material was tested 1 time per and 5 replicates per day.

Multi-site study		
Myoglobin Neo [ng/mL]	Reproducibility	
	AVG [ng/mL]	CV (%)
55	54.57	5.72
100	98.94	6.05
300	301.38	5.89

■ Accuracy


The accuracy was confirmed by testing with 3 different lots of **ichroma™ Myoglobin Neo**. The tests were repeated 10 times at each concentration of the control standard.

Myoglobin Neo [ng/mL]	Lot 1	Lot 2	Lot 3	AVG [ng/mL]	Recovery (%)
5.00	5.33	5.41	5.35	5.36	107%

104.00	106.83	104.59	104.68	105.37	101%
203.00	195.67	199.02	203.71	199.47	98%
302.00	310.21	288.08	301.43	299.91	99%
401.00	406.12	397.72	393.41	399.08	100%
500.00	480.81	467.81	471.21	473.28	95%

■ Comparability

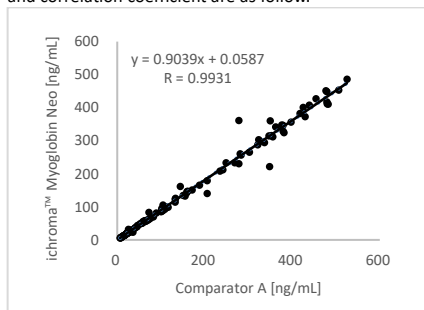











Myoglobin concentration of 120 clinical samples were quantified independently with **ichroma™ Myoglobin Neo (ichroma™ II)** and **comparator A** as per prescribed test procedures. Test results were compared, and their comparability was investigated with linear regression and correlation coefficient (R). The regression equation and correlation coefficient are as follow.



REFERENCES

1. C. Daniel Cabaniss, Creatine Kinase, in: H.K. Walker, W.D. Hall, J.W. Hurst (Eds.), Clinical Methods: The History, Physical, and Laboratory Examinations, 3rd Ed., Butterworths, Boston, 1990, pp 161-163.
2. Adams, J.E., Abendschein, D.R., Jaffe A.S., Biochemical markers of myocardial injury: Is MB creatine kinase the choice for the 1990s, Circulation, 1993; 88: 750-63.
3. Kent Lewandowski, Ahchean Chen and James Januzzi, Cardiac markers for myocardial infarction, Am J Clin Pathol 2002;118 (Suppl 1):S93-S99.
4. Analysis of creatine kinase, CK-MB, myoglobin, and troponin T time- activity curves for early assessment of coronary artery reperfusion after intravenous thrombolysis Circulation. 1993;87:1542-1550.
5. Simultaneous Rapid Measurement of Whole Blood Myoglobin, Creatine Kinase MB, and Cardiac Troponin I by the Triage Cardiac Panel for detection of Myocardial Infarction Clinical Chemistry 45:2 199–205 (1999).
6. Diagnostic Marker Cooperative Study for the Diagnosis of myocardial Infarction Circulation. 1999;99:1671-1677
7. Bedside Multimarker Testing for Risk Stratification in Chest Pain Units: The Chest Pain Evaluation by Creatine Kinase-MB, Myoglobin, and Troponin I (CHECKMATE) Study Circulation. 2001;103:1832-1837

Note: Please refer to the table below to identify various symbols

	Sufficient for <n> tests
	Read instruction for use
	Use by Date
	Batch code
	Catalog number
	Caution
	Manufacturer
	Authorized representative of the European Community
	In vitro diagnostic medical device
	Temperature limit
	Do not reuse
	This product fulfills the requirements of the Directive 98/79/EC on in vitro diagnostic medical devices

For technical assistance, please contact:

Boditech Med Inc.'s Technical Services

Tel: +(82) -33-243-1400

E-mail: TS@boditech.co.kr



Boditech Med Inc.

43, Geodudanji 1-gil, Dongnae-myeon, Chuncheon-si,

Gang-won-do, 24398, Republic of Korea

Tel: +(82) -33-243-1400

Fax: +(82) -33-243-9373

www.boditech.co.kr



Obelis s.a

Bd. Général Wahis 53, 1030 Brussels, Belgium

Tel: +(32) -2-732-59-54

Fax: +(32) -2-732-60-03

E-Mail: mail@obelis.net

