Test Components

This is not a complete Instruction for use. For more detailed instructions, please refer to IFU.

Free PSA\_Rev00\_230612E

Shake 20 times.



Test cartridge



Detector tube (Granule)



Detector diluent



Capillary tube



Ensure that the lot number of the components match.

LOT Matches LOT

If extraction buffer tube are stored in refrigerator, keep the sample collection tube at room temperature for 30 minutes just prior to the test.


Just right Too little or Builded in the sample collection tube at room temperature for 30 minutes just prior to the test.


## **Test Procedure**


- 1 Draw 150 μL. (Detector diluent)
- Add it into detector tube.

  \* Use within 30 seconds.



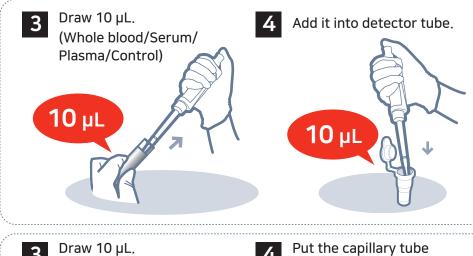



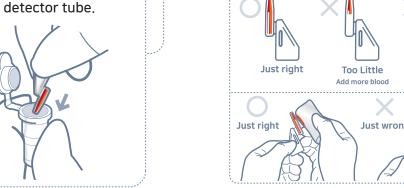






(whole blood)







Too much











